App No.: Not Yet Assigned   Docket No.: HO-P02680US1
Inventor: William A. Zoghbi et al.
Title: USE OF BNP DURING STRESS TESTING FOR THE
DETECTION AND RISK STRATIFICATION OF INDIVIDUALS
WITH SUSPECTED CORONARY ARTERY DISEASE
Sheet 1 of 2

1/2

Change in BNP from Baseline to Immediate Post Ex in Patients With and Without Ischemia
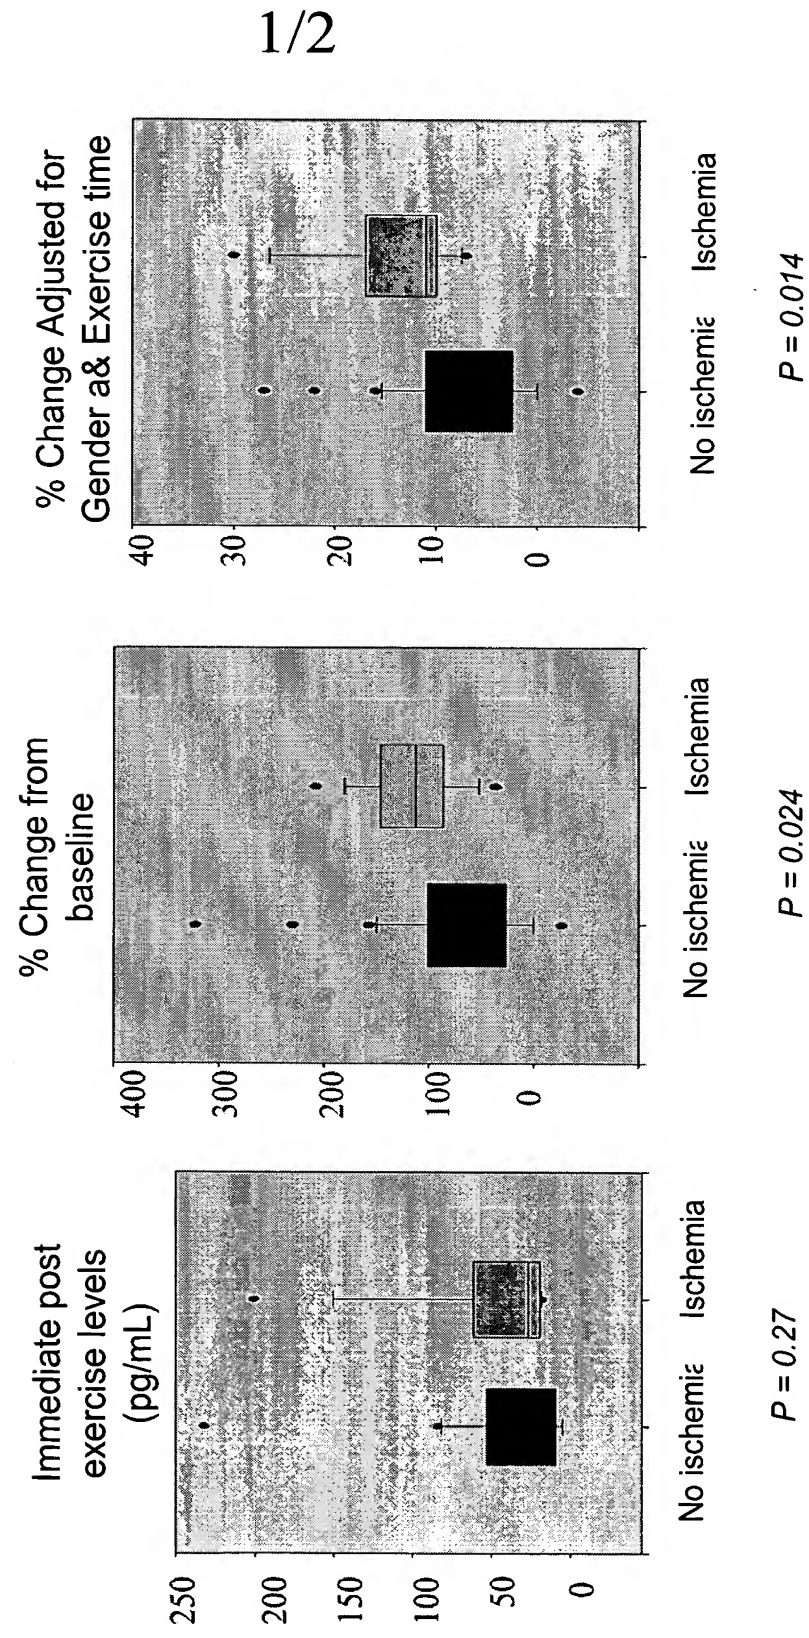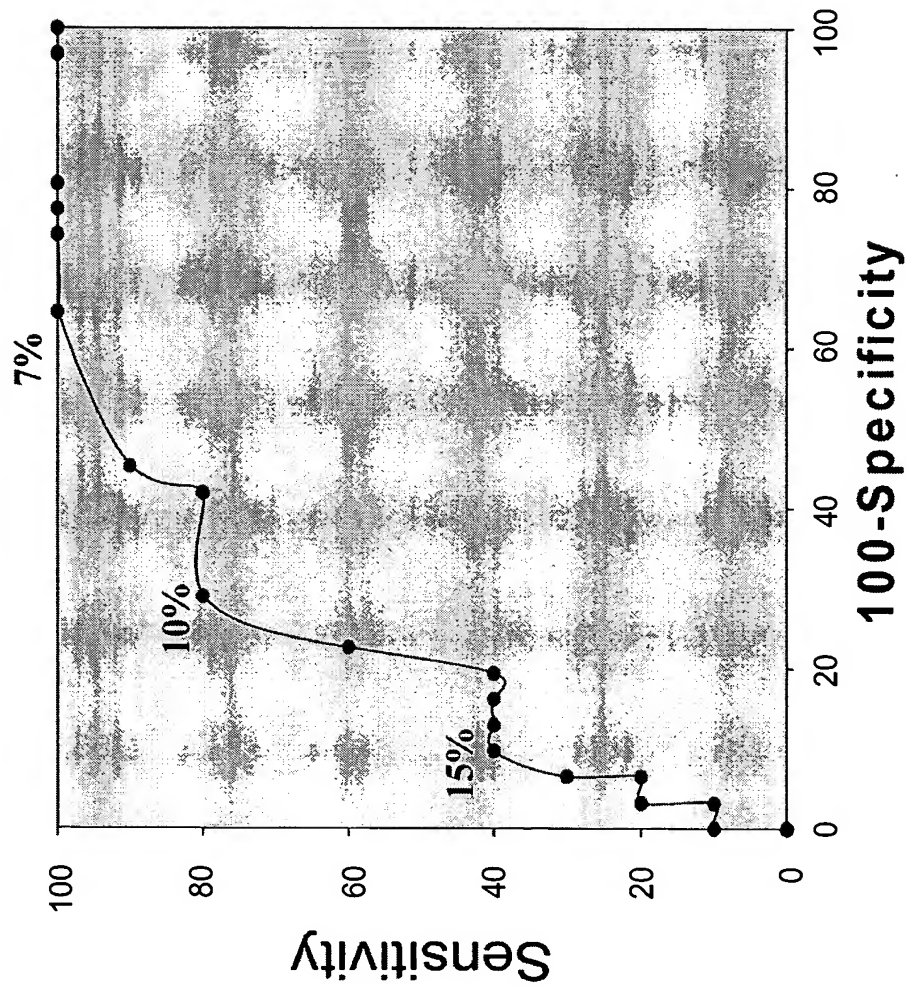
FIG.1

App No.: Not Yet Assigned   Docket No.: HO-P02680US1
Inventor: William A. Zoghbi et al.
Title: USE OF BNP DURING STRESS TESTING FOR THE
DETECTION AND RISK STRATIFICATION OF INDIVIDUALS
WITH SUSPECTED CORONARY ARTERY DISEASE
Sheet 2 of 2

2/2

Prediction of Reversible Ischemia on SPECT by
%Change in BNP Adjusted for Gender and Exercise Time

FIG.2

Area under the ROC Curve = 0.797
Standard error   = 0.091
95% Confidence interval = 0.642 to 0.906